1 Mains Filter

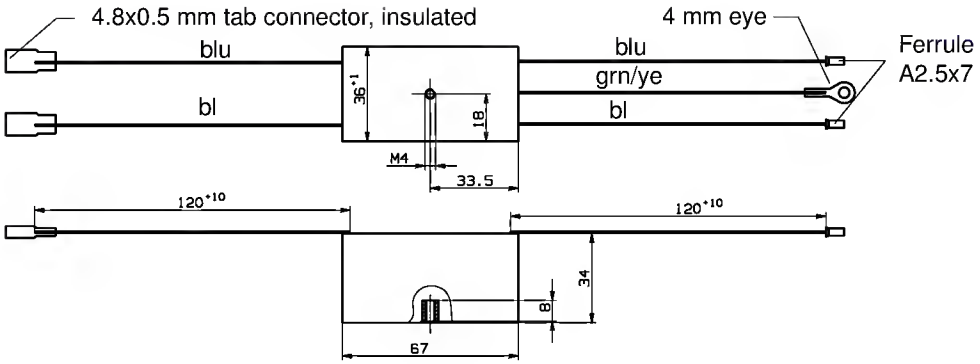

Technical data:

- Rated voltage 240 V (50/60 Hz)
- Nominal current 15 A (40 °C)
- Conductor area 1.5 mm^2 or AWG 14
- Leakage current < 0.25 mA, operating state
  < 0.5 mA, first-fault condition
  see EN 60601-1 Clause 19
- Electrical components, cables, printed board
  Encapsulated with UL- or CSA approval for and system voltage use

IEC heating appliance built-in connector
Supplier: Schurter
Order code: 6110.3300
Enclosed, loose

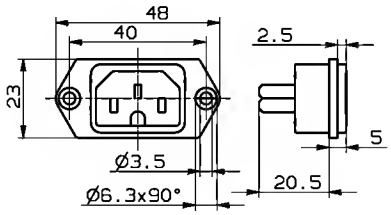

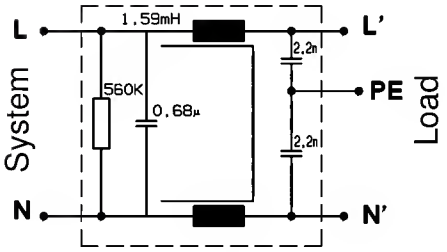

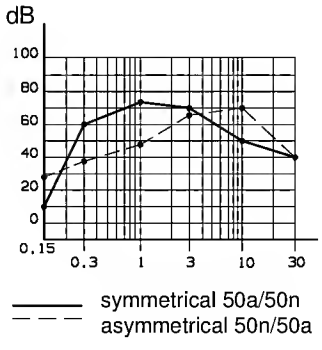

Fig. 1: Babytherm mains filter

GBS6132300T02.fm 15.09.99
For internal use only. Copyright reserved.

2 Mains Voltage Distributor

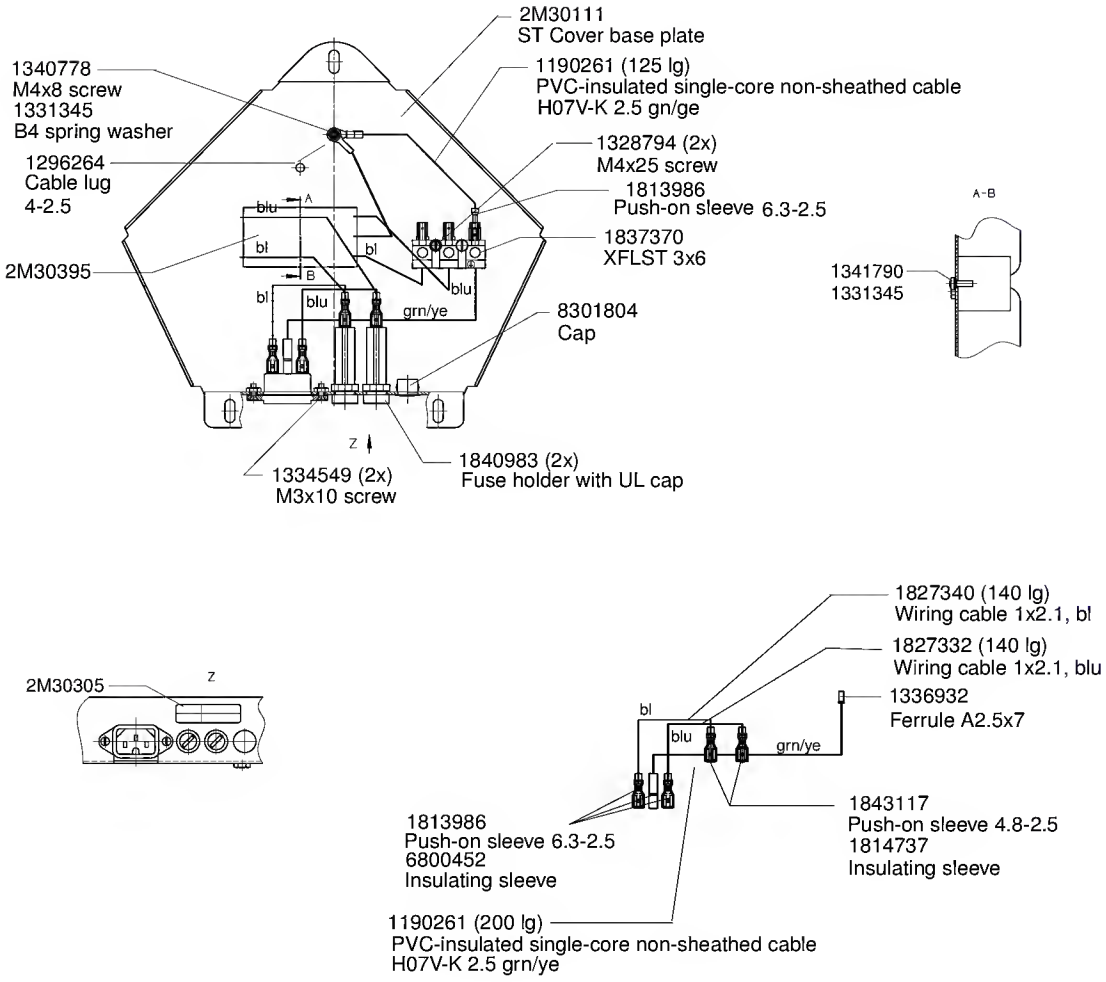

Fig. 2: Mains voltage distributor

GBS6132300T02.fm 15.09.99
For internal use only. Copyright reserved.

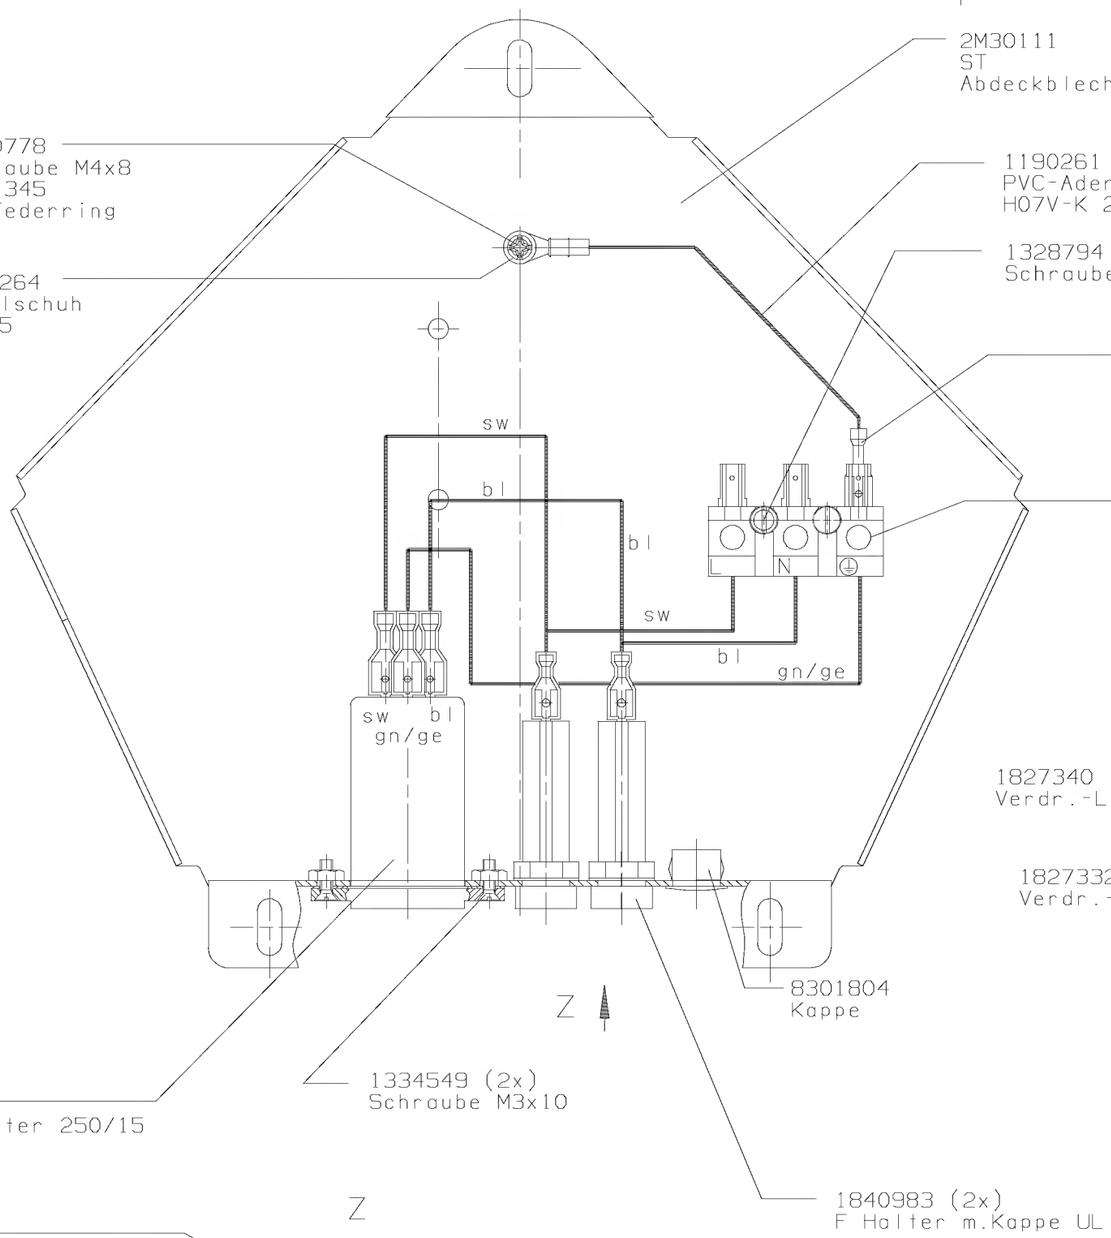

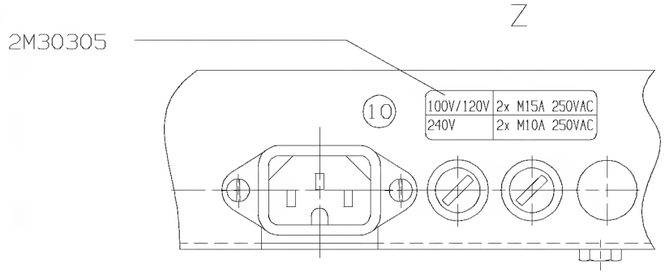

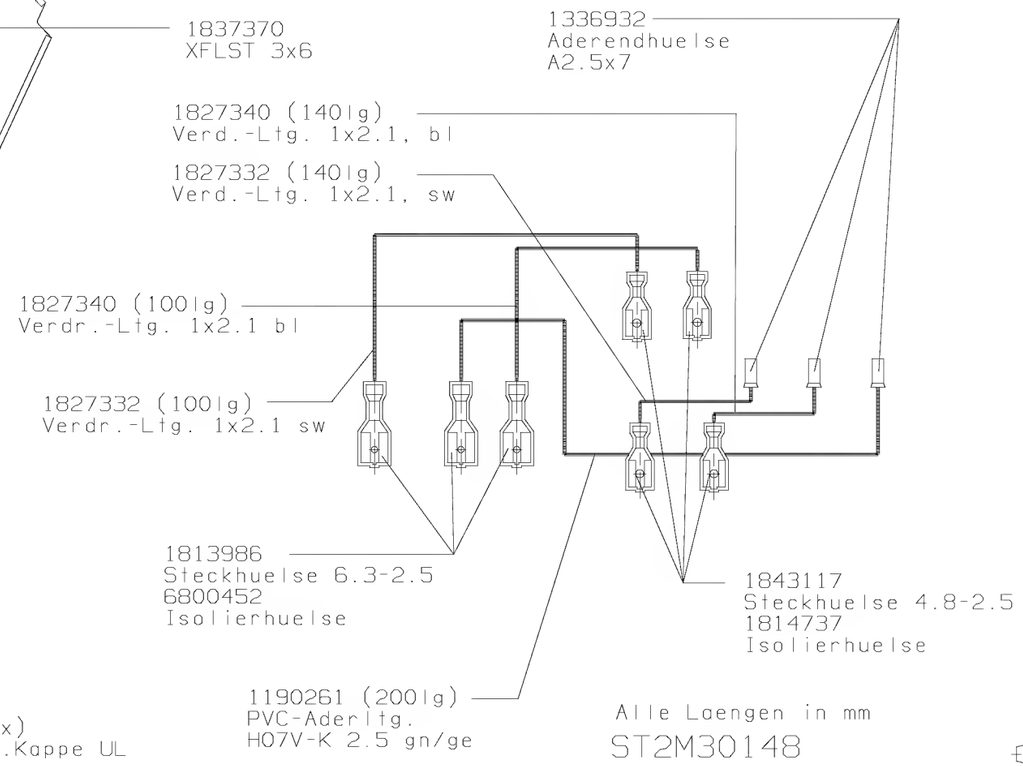

Alle Laengen in mm

ST2M30148

Schutz nach DIN 34 beansprucht.
Weitergabe sowie Vervielfältigung dieser Unterlage, Verwertung und Mitteilung ihres Inhalts nicht gestattet, soweit nicht ausdrücklich zugestanden.
This document, contents or parts thereof are not to be passed on or reproduced, used or communicated without express authority.
Offenders are liable to damages.
All rights reserved.
Dräger Medizintechnik GmbH, D-23542 Lübeck

scale: ---	general tolerances: ---	material: ---	safety class: <s> 0 <m> 0	
field reserved	revision text: Darstellung Schild geaendert (1998/OC/169)			
filing dept.: 2530	responsible dept.: 3401	author: Stickel	approved: Hartwig	contract: ⊓
		date: 04.08.1998	04.08.1998	
type: drawing	language: de	title: Netz Basisplatte		
	replacement for: 2M30148-09	number: 2M30148		
creating system: CADRA	release status: PROD	revision index: 10	accures: 1x	page/of: 01/01

Dräger Medizintechnik GmbH, D-23542 Lübeck

size A2